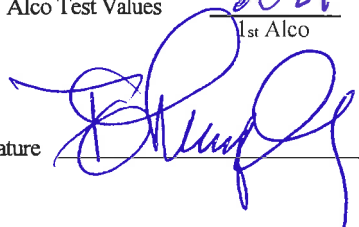


VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm Breath Test Instrument
State of Alaska*


Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

| | | |
|---|-----------------------------|------------------------------------|
| Supervisor/Operator Performing the Verification Procedure: | | DataMaster cdm S/N <u>130192</u> ✓ |
| Name <u>TRACEY MURPHY</u> | ID# <u>7152</u> ✓ | Date <u>12-2-10</u> ✓ |
| A Agency <u>JUNEAU POLICE DEPT</u> | Phone # <u>907 586 0600</u> | |
| Instrument Location <u>JUNEAU POLICE DEPT</u> | | |
| B Alco S/N <u>77621</u> ✓ Target Value <u>0.079</u> ✓ High Pressure <u>30.35</u> | | |
| Alco Test Values <u>0.081</u> ✓ <u>0.081</u> ✓ 1st Alco 2nd Alco | | |
| Signature  | | |
| (OVER) | | |


(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

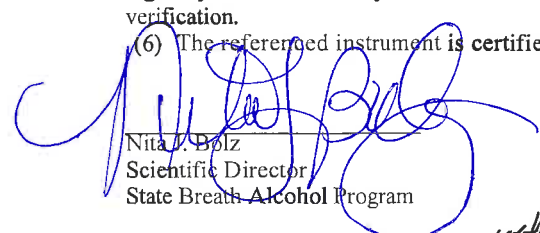
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 10th day of DEC, 2010.


(Notary Seal Stamp)
Daniel L. Nicholas
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130192

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130192

DECEMBER 02, 2010

OPERATOR'S NAME:

MURPHY/TRACY/ERNEST

OPERATOR'S NUMBER: 7252

SUBJECT'S LAST NAME:

MURPHY

SUBJECT'S FIRST NAME/MI :

TRACY/E

O.L. #: VOC

DEPT/AGENCY: JNU1

CASE/REPORT: VOC

TEST TYPE: V

ALCO TARGET VALUE: .079

ALCO S/N: 77621

--- BREATH ANALYSIS ---

.079 ADJUSTED FOR 30.35 in

ALCO TARGET .080 16:04

BLANK TEST .000 16:05

INTERNAL STANDARD VERIFIED 16:05

ALCO TV 30.35 in .081 16:06

BLANK TEST .000 16:06

SUBJECT SAMPLE .000 16:07

BLANK TEST .000 16:08

ALCO TV 30.35 in .081 16:08

BLANK TEST .000 16:09

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130192

DECEMBER 02, 2010

TIME 15:59

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 42c

BAROMETER: 30.35 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY